
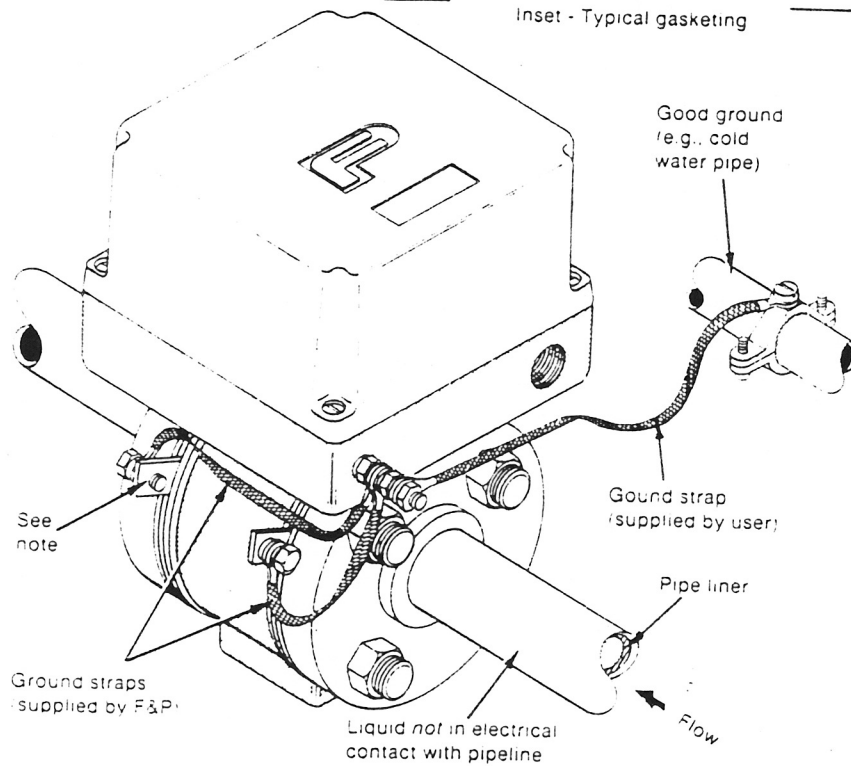


(A) Non-insulated pipe

FIGURE 11-14
Pipe installations.
 (Courtesy Fischer & Porter Company)

Note:
Metal ring in contact with liquid (supplied by user). A quantity of 4 gaskets are needed for proper installation of the 2 grounding rings required (see inset). When the grounding rings are purchased from F&P, gaskets are supplied.

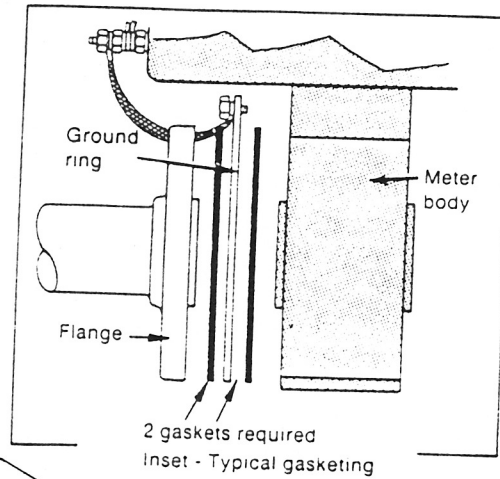

(B) Insulated pipe

FIGURE 11-14
(continued)